


## Advancing OR Safety


### Adhesive Patient Return Electrode

Current flows from patient to a **small surface area** of the sticky pad **allowing** high current concentration

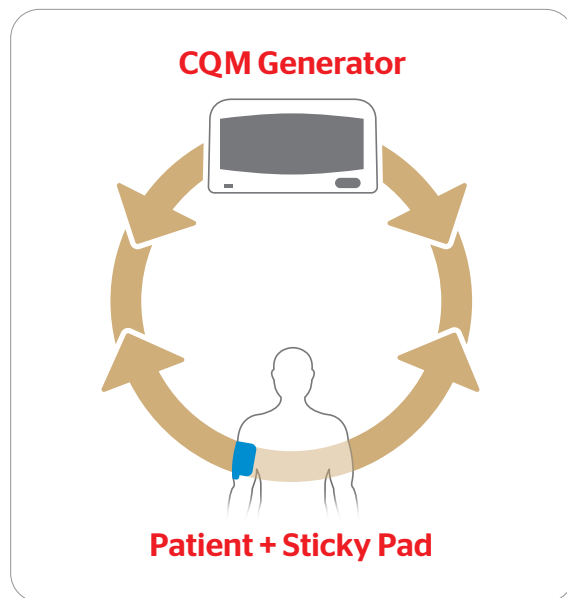


### MEGADYNE™ MEGA SOFT™

Current flows from patient to a **large surface area** of the MEGA SOFT™ **preventing** high current concentration

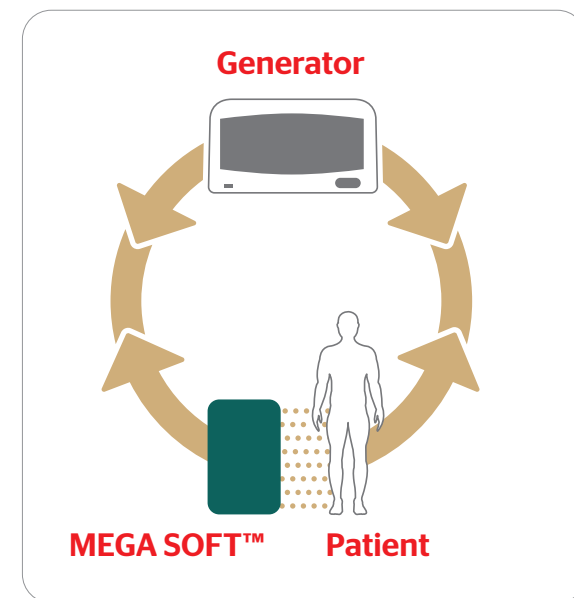

## Adhesive Patient Return Electrode


Current flows from patient to a **small surface area** of the sticky pad **allowing** high current concentration

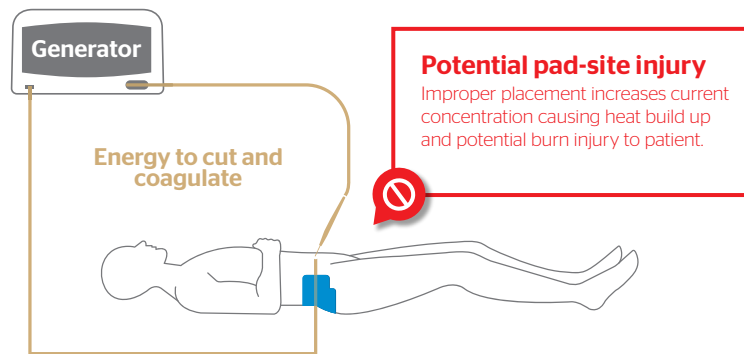

- Potential for pad-site injury
- Direct skin contact needed for current to return to the generator
- Small surface area to disperse current
- Single use

## MEGADYNE™ MEGA SOFT™

Current flows from patient to a **large surface area** of the MEGA SOFT™ **preventing** high current concentration

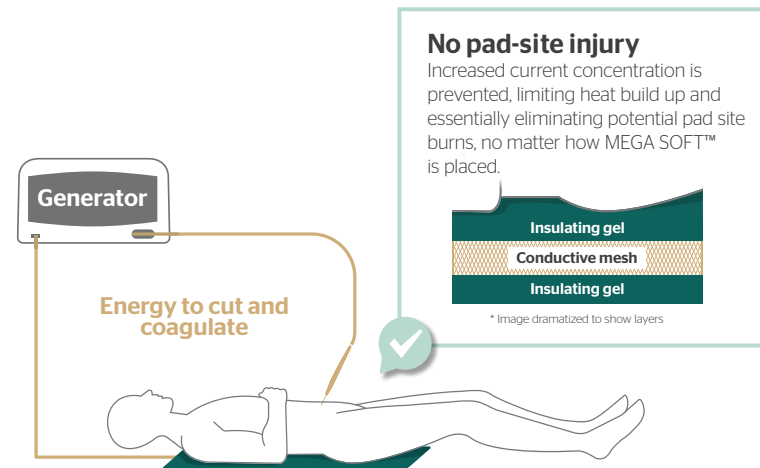

- No heat build-up at MEGA SOFT™ / patient interface
- No direct contact needed
- Large surface area to disperse current
- Reusable up to 24 months<sup>1</sup>

1. Compared to traditional "sticky" patient return electrode. (074679-170614)

Please refer always to the Instructions for Use / Package Insert that come with the device for the most current and complete instructions.