



PARTIAL TEAR. COMPLETE SOLUTION.

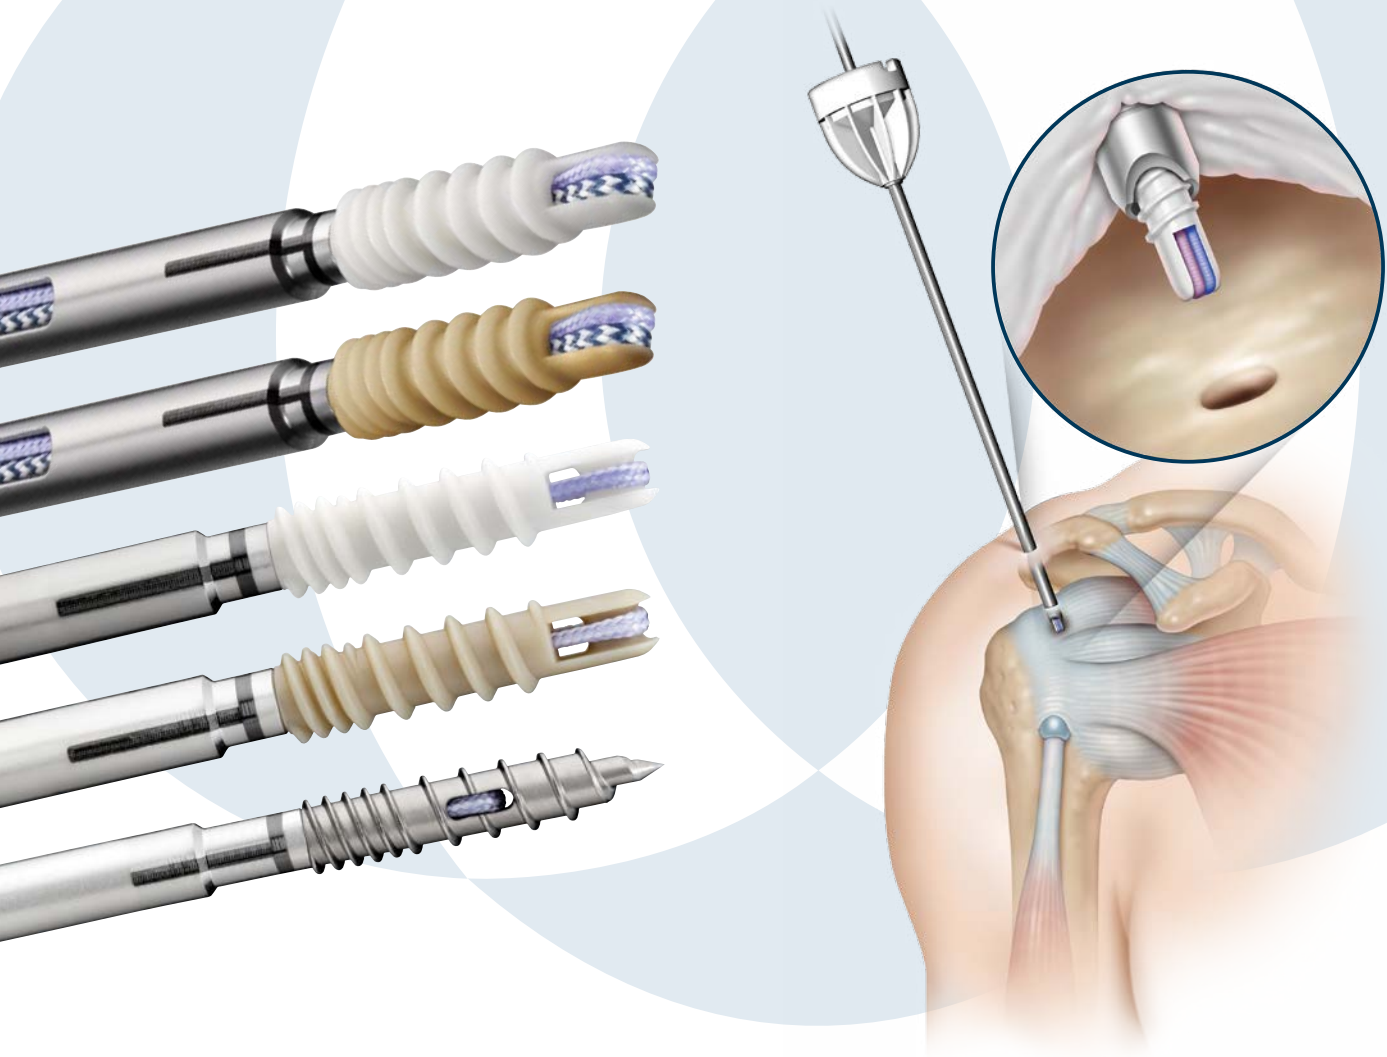

*Getting your patients back to
their passion is our passion.*



HEALIX TRANSTEND™
Implant System

COMPREHENSIVE SOLUTION FOR PARTIAL ROTATOR CUFF TEARS

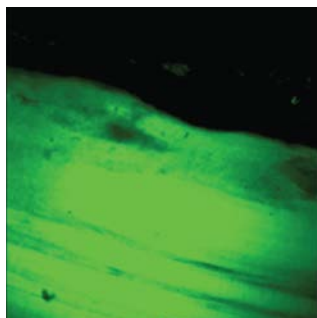

"The HEALIX TRANSTEND™ Implant System, among the anchors tested, caused the least damage to the tendon tissue."¹

- Cortical and cancellous threads for optimum bone bite
- Small diameter for exact placement
- Cannulated anchor to channel blood to surface

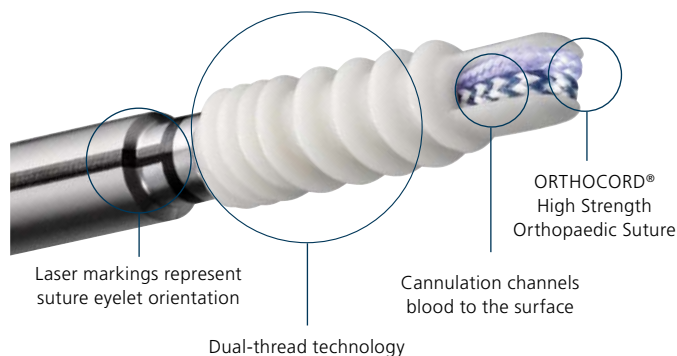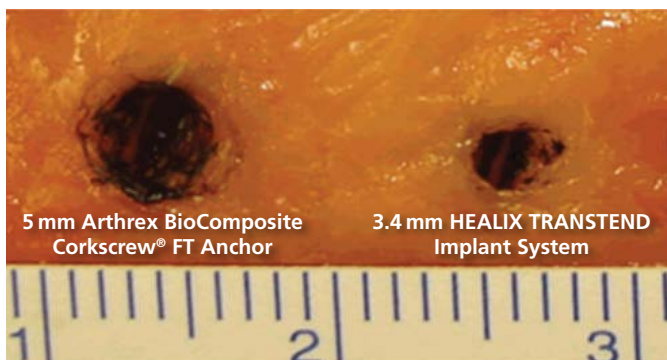

Minimized trauma to surrounding tissue

Ordering Information

CATALOG NUMBER	DESCRIPTION
HEALIX TRANSTEND PEEK Implant System (3.4mm Anchor, #2 ORTHOCORD® Suture)	
222276	HEALIX TRANSTEND PEEK Anchor with Violet Suture
222278	HEALIX TRANSTEND PEEK Anchor with Violet Suture and PERCANNULA™ System
222280	2 HEALIX TRANSTEND PEEK Anchors with Violet Suture and PERCANNULA System
222342	HEALIX TRANSTEND PEEK Anchor with Blue Suture
222340	2 HEALIX TRANSTEND PEEK Anchors with Violet and Blue Suture and PERCANNULA System
222339	HEALIX TRANSTEND PEEK Anchor, Double-Loaded Violet/Blue Suture and PERCANNULA System
HEALIX TRANSTEND Ti Implant System (2.9mm Anchor, #2 ORTHOCORD Suture)	
222260	HEALIX TRANSTEND Ti Anchor with Violet Suture
222266	HEALIX TRANSTEND Ti Anchor with Violet Suture and PERCANNULA System
222268	2 HEALIX TRANSTEND Ti Anchors with Violet Suture and PERCANNULA System

CATALOG NUMBER	DESCRIPTION
HEALIX TRANSTEND BR™ Implant System (3.4mm Anchor, #2 ORTHOCORD Suture)	
222265	HEALIX TRANSTEND BR Anchor with Violet Suture
222261	HEALIX TRANSTEND BR Anchor with Violet Suture and PERCANNULA System
222263	2 HEALIX TRANSTEND BR Anchors with Violet Suture and PERCANNULA System
222341	HEALIX TRANSTEND BR Anchor with Blue Suture
222338	2 HEALIX TRANSTEND BR Anchors with Violet and Blue Suture and PERCANNULA System
222337	HEALIX TRANSTEND BR Anchor, Double-Loaded Violet/Blue Suture and PERCANNULA System
Instrumentation and Disposables	
222274	PERCANNULA System (cannulated obturator, 4mm cannula and 1.1mm guidewire)
222273	HEALIX TRANSTEND Anchor Awl/Tap, 3.4mm (BR and PEEK)
222281	HEALIX TRANSTEND Anchor Drill Bit, 2.2mm (optional for Ti)



DePuy Mitek, Inc.
 325 Paramount Dr.
 Raynham, MA 02767
 USA
 Tel: +1 (800) 382-4682

www.depuyssynthes.com

The third-party trademarks used herein are trademarks of their respective owners.
 © DePuy Synthes Mitek Sports Medicine, a division of DOI 2016. All rights reserved.
 DSUS/MTK/0416/0767 5/16

References

1. Zhang QS, Liu S, Zhang Q, Xue Y, Ge D, O'Brien MJ, Savoie FH, You Z. Comparison of the Tendon Damage Caused by Four Different Anchor Systems Used in Transtendon Rotator Cuff Repair. Products tested include: HEALIX PEEK™ Anchor, FASTIN® RC Threaded Anchor, HEALIX TRANSTEND Anchor and Arthrex BioComposite Corkscrew FT Anchor